



Comparison with another electrolyte analyser

a. Instrument A


(Na)

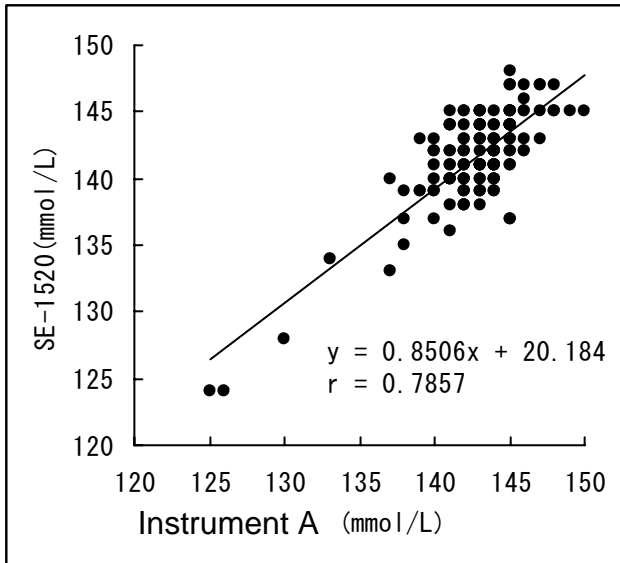

(K)

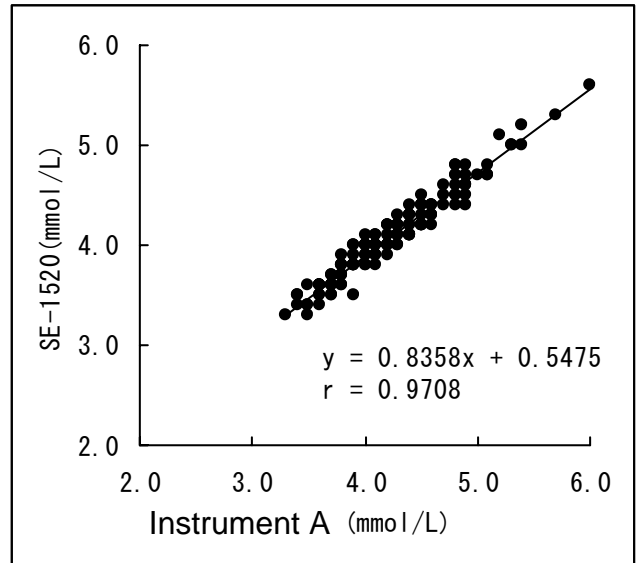


(Cl)

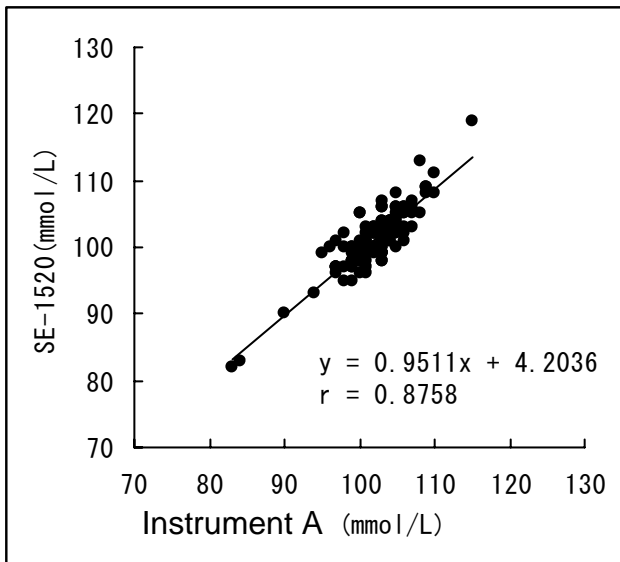


b. Instrument B

(Na)

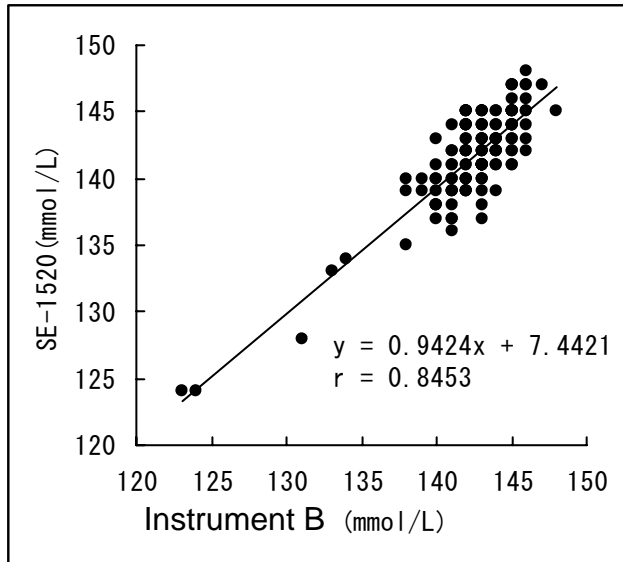

(K)

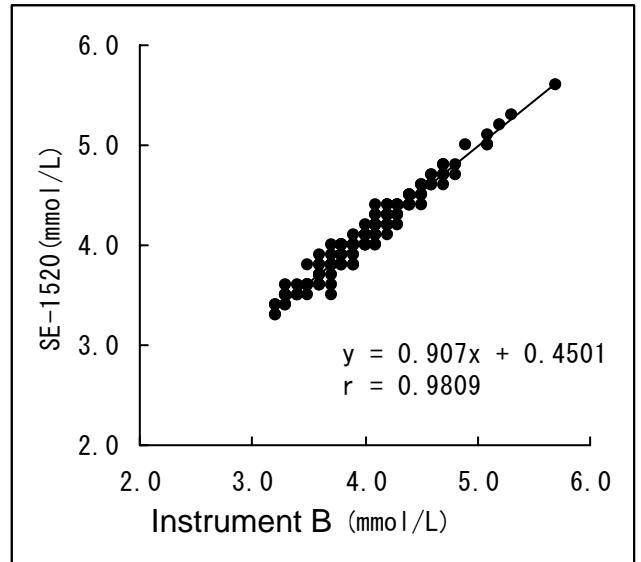

(Cl)

